MANI® Trocar Kit

Trocar

Product Name	Packaging	Color Coding	Order #
Trocar 27G S NEW	6 Pcs./ Box		MTR27S
Trocar 25G S	6 Pcs./ Box		MTR25S
Trocar 23G S	6 Pcs./ Box		MTR23S

* Individually packed – ideal for backup

Infusion Cannula

Product Name	Packaging	Color Coding	Order #
Infusion Cannula 27G S NEW	6 Pcs./ Box		MIC27S
Infusion Cannula 25G S	6 Pcs./ Box		MIC25S
Infusion Cannula 23G S	6 Pcs./ Box		MIC23S

* Individually packed – ideal for backup

Trocar Kit

Product Name	Packaging	Color Coding	Order #
Trocar Kit 27G S NEW	3 Kits/ Box		MTK27S
Trocar Kit 25G S	3 Kits/ Box		MTK25S
Trocar Kit 23G S	3 Kits/ Box		MTK23S

MANI, INC.

8-3 Kiyohara Industrial Park,
Utsunomiya, Tochigi, 321-3231 JAPAN
TEL: +81.28.667.7565 / FAX: +81.28.667.8305
URL: http://www.mani.co.jp/en/
E-mail:seg-ovs@ms.mani.co.jp

Distributed by

Crestpoint Ophthalmics
9100 Watson Rd.
St. Louis, MO 63126 Phone: (314) 849-7773
Email: custsvc@crestpointmgt.com
Website: www.crestpointophthalmics.com

S00760 (230116)

MANI®

Crestpoint OPHTHALMICS

MANI® Trocar Kit

Trocar • Infusion Cannula • Trocar Kit

MANI® Trocar Kit

Ultimate Sharpness, Minimal Stress

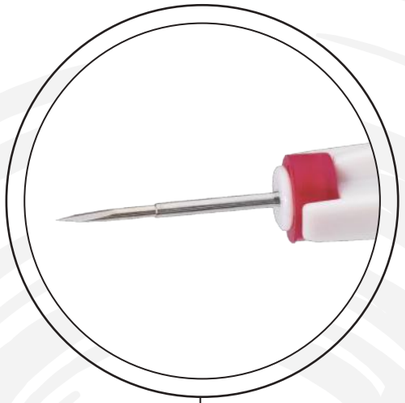

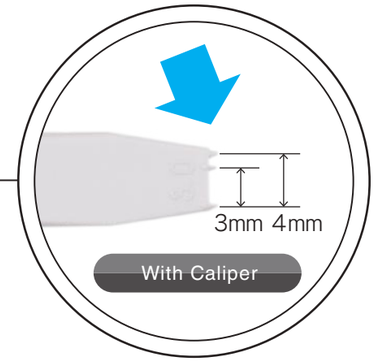

≫ Infusion Cannula

Easily connected without valve removal

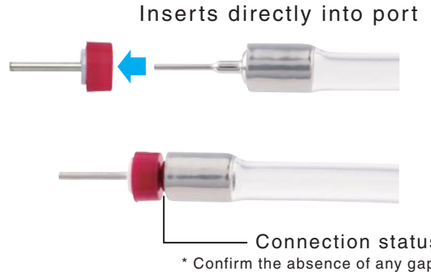

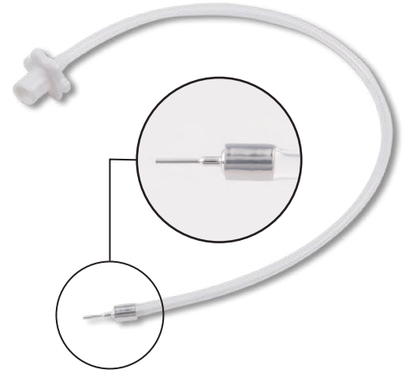

≫ Trocar

Expanded product line.
Individually packed items reduce waste and are ideal as a backup.

Actual size

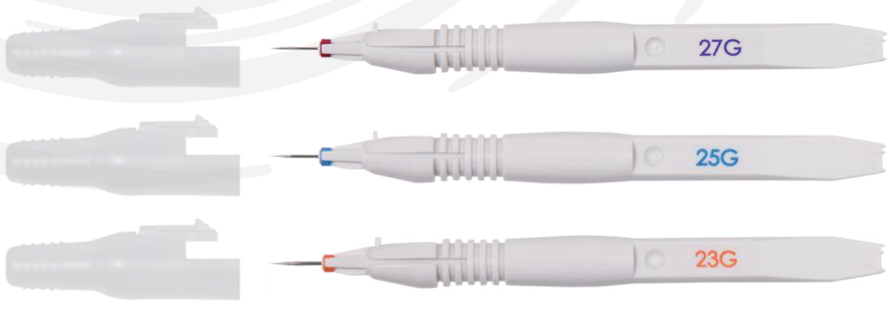

NEW
MTR27S
MTR25S
MTR23S

≫ Trocar Kit

1 Surgery Case (1 Pack)

- Trocar × 3 Pcs.
- Infusion Cannula × 1Pc.

* Individually packaged trocars (shown in the left page) are available for use as a fourth port or as a backup.

■ When holding the cannula

This product can be inserted into the sclera without holding the valved cannula. Withdraw the trocar handle after scleral placement. If the valved cannula does not detach easily, withdraw the trocar handle while gently holding the cannula with fine forceps. Take care not to touch the stop at the end of the handle as shown in the figure at right then position the cannula.